

InBody



InBody270s

Body Composition Analyzer for All

A Body composition analyzer designed for everyday use by everyone

New Standard of BIA

Redefine the depth of health assessment with the Phase Angle

Streamlined Portability


Compact and foldable design to ensure effortless mobility

InBody Technology

InBody uses Bioelectrical Impedance Analysis (BIA) technology to measure human body composition. Impedance is the resistance of the human body generated when a micro alternating current flows through the human body. The human body is made of water that conducts electricity well, and the resistance varies depending on the amount of water. BIA is a technology that quantitatively measures body water through impedance that occurs when an electric current flows through the human body. InBody provides diverse information on body composition based on the measured body water.

Direct Segmental Measurement-BIA

The human body exhibits varying lengths and cross-sectional areas for each body segments. Arms and legs, characterized by narrow cross-sectional areas and length, exhibit higher impedance values and lower muscle mass. Conversely, the trunk, with its broader cross-sectional area, yields lower impedance values and higher muscle mass. Even the slightest change in trunk impedance can significantly influence the total muscle mass. Therefore, it is essential to separately measure trunk impedance for precise total muscle mass assessment. InBody conducts separate measurements for arms, legs, and the trunk, ensuring the utmost accuracy in the analysis.

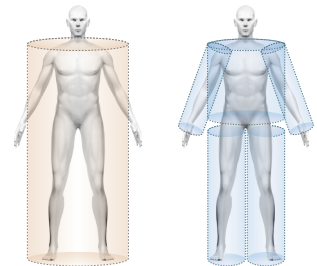


8-Point Tactile Electrodes Utilizing Thumb Electrodes

Using the structural features of the human body, InBody pioneered '8-Point Tactile Electrode with Thumb Electrodes'. This ensures InBody measurements start at the same location on the wrists and ankles, guaranteeing reliable and reproducible results.




Simultaneous Multi-Frequency Impedance Measurement

InBody introduced a technology in body composition analyzers to transmit multiple frequencies at once, obtaining specific impedance data for each for the first time. This reduces measurement time and error, leading to more accurate body water and fluid balance measurements.




No Estimations or Empirical Estimation on Measured Values

InBody does not rely on empirical estimations based on age, gender, and more to ensure the accuracy of the measured data. In the past, empirical estimations were applied to the equations to ensure accuracy due to technological limitations. However, this resulted in lower accuracy when the measured population group changes. InBody overcame these limitations with technological developments such as direct segmental measurement-BIA to measure and analyze accurate body composition without applying empirical estimation. Therefore, InBody devices can provide data regardless of population and can reflect changes in the body with higher sensitivity.



Over 98 % Correlation to DEXA on Accuracy

InBody precisely detects changes in body composition using impedance alone, showing a correlation over 0.98 with the gold-standard DEXA device.

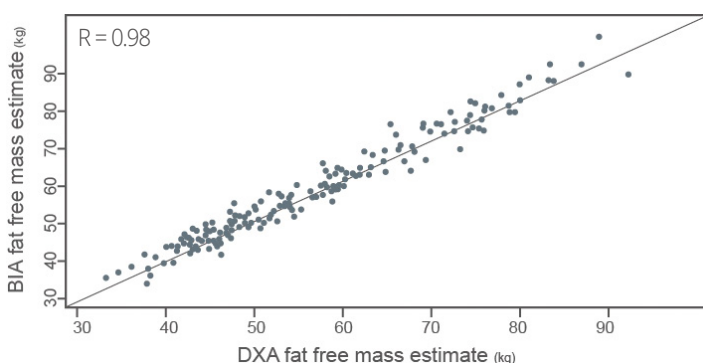

Ryan T Hurt et al., The Comparison of SMF-BIA and DEXA for Estimating Fat Free Mass and Percentage Body Fat in an Ambulatory Population, *J Parenter Enteral Nutr.*, 2021 Aug;45(6):1231-1238

InBody270S Highlights

Quick Measurement

Experience InBody's quick and precise measurement in only 30 seconds, with ensured reliability. Users can access their health data instantly, facilitating prompt consultations.

Compact and Portable Design

The foldable structure and compact size ensure easy transportation and spatial efficiency. The optional InBody270S carrying bag enhances portability. Its compact size maximizes space utilization without compromising on functionality.

Results in Your Hands

Transfer your body composition data directly to your mobile phone using our QR Code feature. Stay connected and track your progress anytime, anywhere with instant access to your detailed results.



Comprehensive Parameters for All

Nutrition Assessment

In-depth Body Composition Analysis

Nutrition Analysis offers comprehensive evaluations of protein, mineral levels, and body fat to ensure the body's nutritional needs are met for optimal health. By providing insights into protein consumption, mineral status, and Percent Body Fat, it empowers users to make informed dietary choices. With this in-depth analysis, achieving a balanced diet and monitoring progress toward health goals becomes straightforward and manageable.

Cellular Integrity Check

Phase Angle

The human body comprises 36 trillion cells, and understanding cell health is crucial for overall well-being. The Phase Angle is a key parameter in assessing cell health and overall physiological status. It reflects the relationship between resistance in total body water and reactance in cell membrane. A higher Phase Angle indicates better cell membrane integrity, and well-balanced fluid, suggesting healthier cells. Last but not least, with the addition of Whole Body Phase Angle History, users can intuitively track and monitor their health trends over time.

Sarcopenia Assessment

SMI(Skeletal Muscle Mass Index)

Sarcopenia, assigned the diagnosis code M62.84 by the WHO, is recognized as a disease rather than just a natural phenomenon. It can be easily assessed and evaluated using the Skeletal Muscle Mass Index (SMI)* and Hand Grip Strength**, allowing for comprehensive evaluation and personalized consultations.

* Skeletal Muscle Mass Index (SMI) calculated by taking the sum of the Appendicular Muscle Mass (in kilograms) and dividing it by the square of the person's height (in meters).

**Hand Grip Strength is available with connections to the InBody Handgrip Dynamometer (IB-HGS, optional).



InBody Result Sheet

Provides reference parameters to thoroughly evaluate patients' conditions across various medical practices.

InBody

[InBody270S]

7

Customized Logo


www.customized.com

| | | | | |
|----------|---------|-----|--------|------------------|
| ID | Height | Age | Gender | Test Date & Time |
| Jane Doe | 156.9cm | 51 | Female | 05.30.2025 11:16 |


1 Body Composition Analysis

| | | | |
|-------------------------------|-------------------------|------|----------------------|
| Total amount of water in body | Total Body Water | (L) | 28.1 (27.0 ~ 33.0) |
| For building muscles | Protein | (kg) | 7.4 (7.2 ~ 8.8) |
| For strengthening bones | Minerals | (kg) | 2.76 (2.49 ~ 3.05) |
| For storing excess energy | Body Fat Mass | (kg) | 20.8 (10.6 ~ 16.9) |
| Sum of the above | Weight | (kg) | 59.1 (45.0 ~ 60.8) |


2 Muscle-Fat Analysis

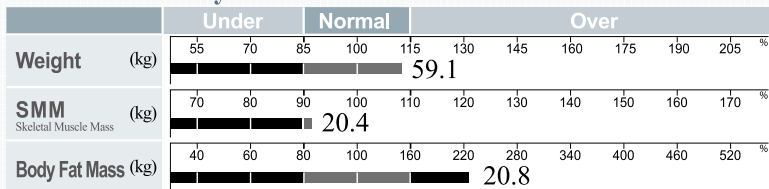


3 Obesity Analysis

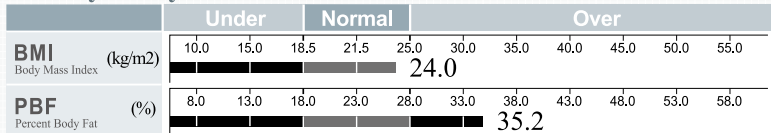

4 Segmental Lean Analysis

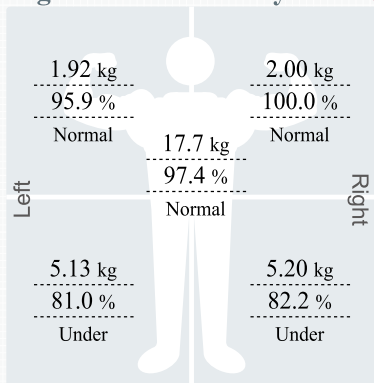

5 Segmental Fat Analysis

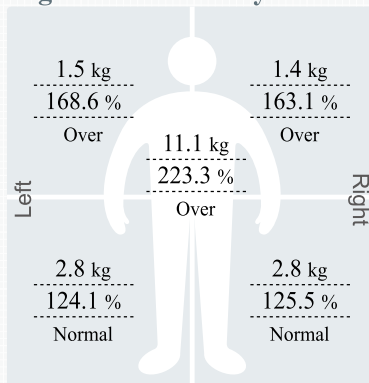

* Segmental fat is estimated.

6 Body Composition History

| | 01.01.25 09:15 | 01.30.25 09:40 | 02.20.25 09:35 | 03.15.25 11:10 | 04.12.25 08:33 | 04.28.25 15:10 | 05.15.25 08:40 | 05.30.25 11:16 |
|-----------------|----------------|----------------|----------------|----------------|----------------|----------------|----------------|----------------|
| Weight | 65.3 | 63.9 | 62.4 | 61.8 | 62.3 | 60.9 | 60.5 | 59.1 |
| SMM (kg) | 20.1 | 20.0 | 19.7 | 19.7 | 19.8 | 19.7 | 19.8 | 20.4 |
| PBF (%) | 41.3 | 40.7 | 39.2 | 39.0 | 39.4 | 38.6 | 37.8 | 35.2 |

Recent Total

8 InBody Score

69 / 100 Points
 * Total score that reflects the evaluation of body composition. A muscular person may score over 100 points.

9 Whole Body Phase Angle

| | | | | | |
|-------------------------|----------------|----------------|----------------|----------------|----------------|
| $\phi(^{\circ})$ 50 kHz | 4.3 ° | | | | |
| | 4.3 | 4.4 | 4.2 | 4.1 | 4.3 |
| | 03.15.25 11:10 | 04.12.25 08:33 | 04.28.25 15:10 | 05.15.25 08:40 | 05.30.25 11:16 |

10 Weight Control

Target Weight 53.0 kg
 Weight Control - 6.1 kg
 Fat Control - 8.6 kg
 Muscle Control + 2.5 kg

11 Waist-Hip Ratio

0.96 0.75 0.85

12 Visceral Fat Level

11 Low 10 High

13 Research Parameters

Fat Free Mass 38.3 kg (36.7 ~ 44.8)
 Basal Metabolic Rate 1197 kcal (1255 ~ 1451)
 Obesity Degree 112 % (90 ~ 110)
 Recommended calorie intake 1397 kcal

Calorie Expenditure of Exercise

| | | | |
|-------------------|-----|--------------|-----|
| Golf | 104 | Gateball | 112 |
| Walking | 118 | Yoga | 118 |
| Badminton | 134 | Table Tennis | 134 |
| Tennis | 177 | Bicycling | 177 |
| Boxing | 177 | Racketball | 177 |
| Mountain Climbing | 193 | Jumping Rope | 207 |
| Aerobics | 207 | Jogging | 207 |
| Soccer | 207 | Swimming | 207 |
| Japanese Fencing | 295 | Racketball | 295 |
| Squash | 295 | Taekwondo | 295 |


*Based on your current weight

*Based on 30 minute duration

14 Sarcopenia Parameters

SMI 5.8 kg/m² (< 5.7)
 HGS 15.8 kg (< 18.0)

15 Impedance

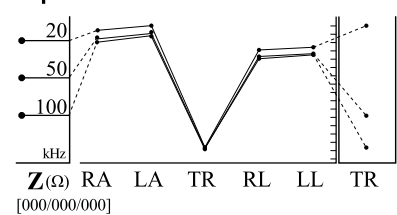

Result Sheet Interpretation

1 Body Composition Analysis

Body weight is the sum of Total Body Water, Protein, Minerals, and Body Fat Mass. Maintain a balanced body composition to stay healthy.

2 Muscle-Fat Analysis

Compare the bar lengths of Skeletal Muscle Mass and Body Fat Mass. The longer the Skeletal Muscle Mass bar is compared to the Body Fat Mass bar, the better health status you are in.

3 Obesity Analysis

BMI is an index used to determine obesity by using height and weight. PBF is the percentage of body fat compared to body weight.

4 Segmental Lean Analysis

Analyze to evaluate if the muscles are adequately developed in the body segments. The top bar shows your muscle mass status compared to the ideal weight and the bottom bar shows your muscle mass status compared to your current weight.

5 Segmental Fat Analysis

Evaluate whether the fat is adequately distributed across the segments of the body. Each bar shows fat mass in comparison to the ideal amount.

6 Body Composition History

Measure your body composition periodically to monitor your progress.

7 Logo Customization

The Customized Logo can be applied on the Result Sheet. URL can also be applied at the bottom of the Result Sheet as well.

8 InBody Score

InBody Score is your score after evaluating your body composition.

9 Whole Body Phase Angle

Phase Angle is related to the health status of the cell membrane. Strengthening of the cellular membrane and structural function will increase the Phase Angle. In contrast, impairments to the cellular membrane can lead to a decrease in Phase Angle.

10 Weight Control

Use the Target Weight, Weight Control, Fat Control, Muscle Control to set your own goal.

11 Waist-Hip Ratio (WHR)

Waist-Hip Ratio is the ratio of waist circumference to hip circumference.

12 Visceral Fat Level

Visceral Fat Level is an indicator based on the estimated amount of fat surrounding internal organs in the abdomen.

13 Research Parameters

Various research parameters such as Basal Metabolic Rate, Waist-Hip Ratio, Obesity Degree, Skeletal Muscle Mass Index (SMI), and more are provided.

14 Sarcopenia Parameters

Sarcopenia is now recognized as a disease. Skeletal Muscle Mass Index (SMI) and Hand Grip Strength (HGS) measurements provide precise assessments for sarcopenia patients, enabling healthcare professionals to develop tailored care plans for effective management.

15 Impedance

Impedance is the resistance value measured when electrical currents are applied to the body. Based on the measured data, key body composition outputs can be analyzed. Impedance is also used for many research purposes.

*Additional InBody Results Sheet

InBody Result Sheet for Children, Thermal Result Sheet

Optional Result Sheet

1 InBody Result Sheet for Children

With the InBody Result Sheet for Children, you can assess and track a child's growth progress.

2 Thermal Result Sheet (Optional)

Thermal Result Sheet is available by connecting the optional TP100 provided by InBody. Parameters on the Thermal Result Sheet are customizable from the InBody device settings.



1 InBody [InBody270S]

| | | | | |
|--------------|---------|-----|--------|------------------|
| ID | Height | Age | Gender | Test Date / Time |
| John Doe Jr. | 139.4cm | 10 | Male | 06.21.2025 16:40 |

Body Composition Analysis

| | | |
|----------------------------------|-----------------------------|----------------------|
| Total amount of water in my body | Total Body Water (L) | 19.2 (18.0 ~ 22.0) |
| What I need to build muscles | Protein (kg) | 5.1 (4.9 ~ 5.9) |
| What I need for strong bones | Minerals (kg) | 1.91 (1.66 ~ 2.04) |
| Where my excess energy is stored | Body Fat Mass (kg) | 8.8 (3.8 ~ 7.7) |
| Sum of the above | Weight (kg) | 35.0 (27.3 ~ 36.9) |

Muscle-Fat Analysis

| | Under | Normal | Over |
|---------------------------|----------|-----------|-----------|
| Weight (kg) | 55 ~ 100 | 100 ~ 160 | 160 ~ 205 |
| SMM (kg) | 70 ~ 100 | 100 ~ 140 | 140 ~ 170 |
| Body Fat Mass (kg) | 40 ~ 80 | 80 ~ 160 | 160 ~ 520 |

Results: Weight 35.0, SMM 13.4, Body Fat Mass 8.8

Obesity Analysis

| | Under | Normal | Over |
|---------------------------------|------------|-------------|-------------|
| BMI (kg/m ²) | 7.9 ~ 16.4 | 16.4 ~ 24.2 | 24.2 ~ 30.2 |
| PBF (%) | 0.0 ~ 20.0 | 20.0 ~ 30.0 | 30.0 ~ 50.0 |

Results: BMI 18.0, PBF 25.2

Growth Graph

Height : 50 ~ 75%

Weight : 50 ~ 75%

Body Composition History

| | 09.10.24 | 11.30.24 | 01.02.25 | 06.21.25 |
|-------------|----------|----------|----------|----------|
| Height (cm) | 136.5 | 137.2 | 138.6 | 139.4 |
| Weight (kg) | 35.1 | 35.6 | 37.3 | 35.0 |
| SMM (kg) | 13.3 | 13.0 | 12.9 | 13.4 |
| PBF (%) | 26.2 | 26.5 | 26.0 | 25.2 |

2 InBody 05/30/2025 11:16

ID : Jane Doe
Height : 156.9cm Age : 51
Gender : Female Weight : 59.1kg

Weight 59.1 kg
Muscle Mass 20.4 kg
Body Fat Mass 20.8 kg
Percent Body Fat 35.2 %
Normal Range (18.0-28.0)

Body Mass Index 24.0 kg/m²
Normal Range (18.5-25.0)

Basal Metabolic Rate 1197 kcal
it is the Minimum number of calories needed to sustain life at a resting state.

Waist Hip Ratio 0.96
Normal Range (0.75-0.85)

Visceral Fat Level 11
Normal Range (1-9)

Segmental Lean Analysis

| | | |
|--------|---------|---------|
| Left | 1.92 kg | 2.00 kg |
| | 95.9 % | 100.0 % |
| Normal | 17.7 kg | Normal |
| Right | 5.13 kg | 5.20 kg |
| | 81.0 % | 82.2 % |
| Under | | Under |

Segmental Fat Analysis

| | | |
|--------|---------|---------|
| Left | 1.5 kg | 1.4 kg |
| | 168.6 % | 163.1 % |
| Over | 11.1 kg | Over |
| Right | 2.8 kg | 2.8 kg |
| | 124.1 % | 125.5 % |
| Normal | | Normal |

* Segmental fat is estimated.

InBody Score 69

Fat Control - 8.6 kg
Muscle Control + 2.5 kg

Whole Body Phase Angle 4.3 °

Impedance

Growth Score 86/100 Points
* If tall and within great body comparison standards, the growth score may surpass 100 points.

Obesity Evaluation
BMI Normal Under Slightly Over Over
PBF Normal Slightly Over Over

Research Parameters
Basal Metabolic Rate 936 kcal (948 ~ 1077)
Child Obesity Degree 109 % (90 ~ 110)


Results Interpretation
Growth Graph
Compares the height and weight among peers of the same age group.

Results Interpretation QR Code
Scan the QR Code to see results interpretation in more detail.

Copyright © 1996-by InBody Co.,Ltd. All rights reserved.

InBody Data Integration Solution

Manage and utilize your InBody data in various settings.

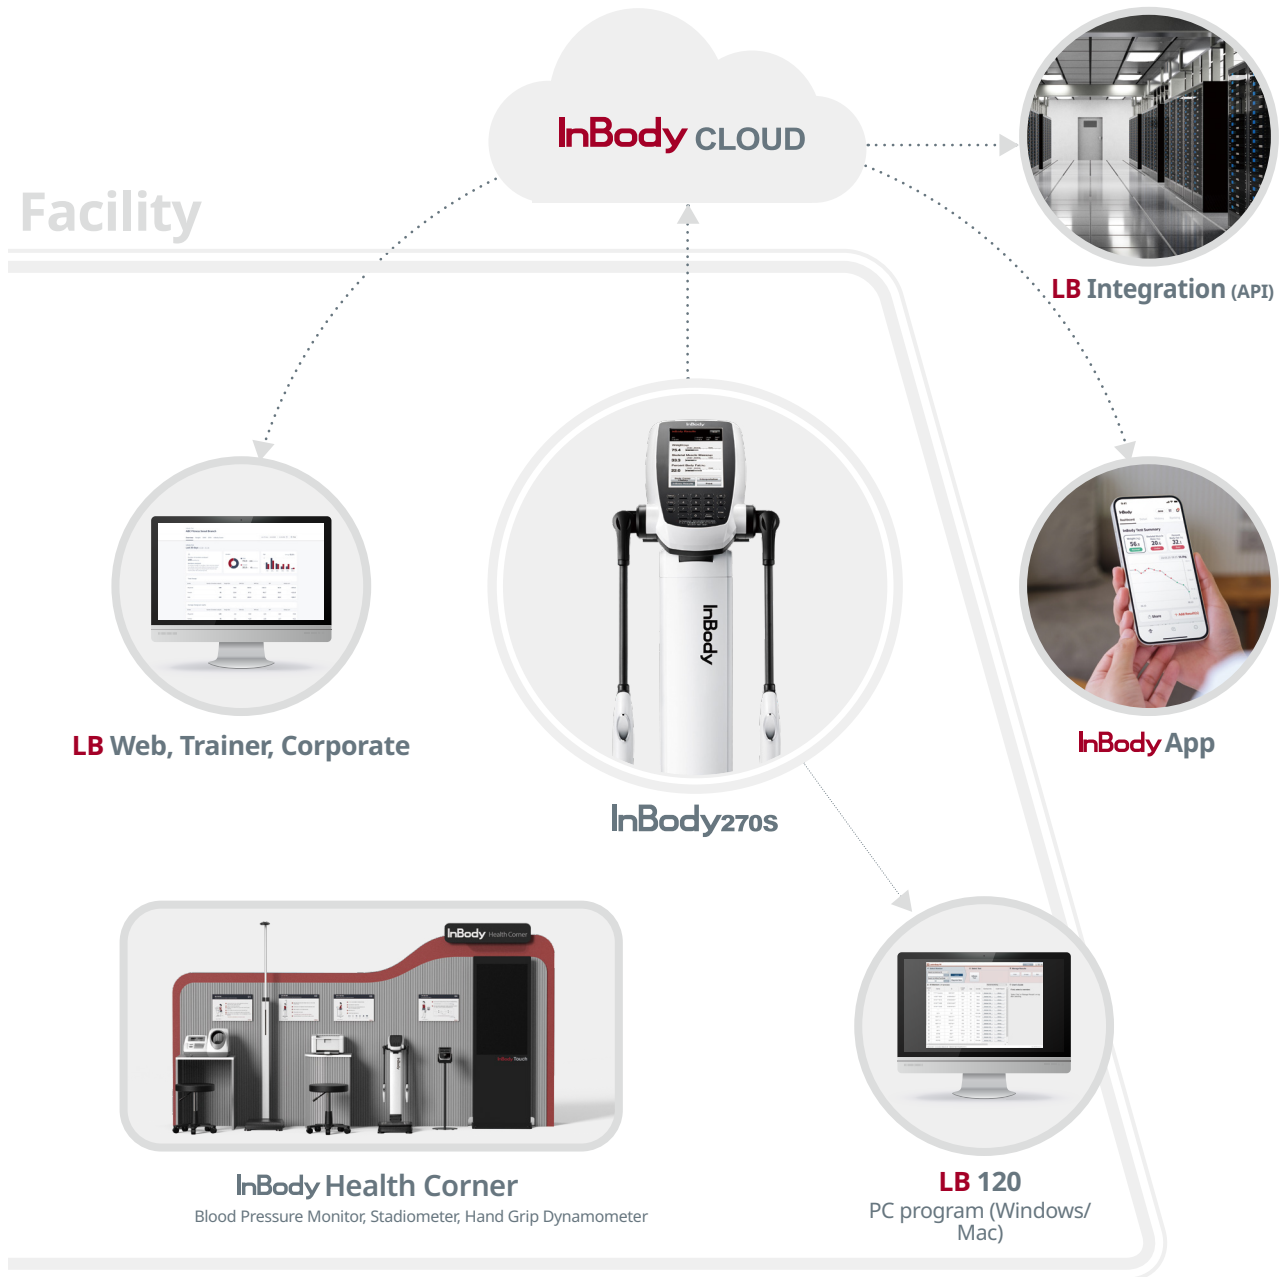

InBody Data Comprehension

Provide a health report to monitor your customers' body composition goals.

Analytical Dashboard and Report

Get an intuitive analysis of your InBody data on the dashboard and see how your facility is performing with InBody.

Monitor Lifestyle Habits

Integrate InBody devices to monitor lifestyle habits and provide remote health management.

Access InBody Results Anywhere, Anytime

Through PC, tablet and smartphones, access your customer's InBody results anywhere, anytime.

API Integration


Upon customer consent, utilize InBody data through API and SDK.

Various File Formats

Print InBody data as an image, excel file etc.

Specifications

InBody270S Body Composition Analyzer

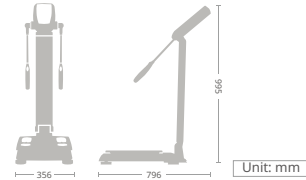

| | |
|---|--|
| Bioelectrical Impedance Analysis (BIA) Measurement Outputs | Impedance (Z) 15 Impedance measurements by using 3 different frequencies (20 kHz, 50 kHz, 100 kHz) at each 5 segments of the body (Right Arm, Left Arm, Trunk, Right Leg, Left Leg) |
| Measurement Method | Phase Angle (Ø) 1 Phase Angle Measurements by Using 1 Frequency (50 kHz) at Whole Body · Direct Segmental Multi-Frequency Bioelectrical Impedance Analysis (DSM-BIA) · Simultaneous Multi-Frequency Bioelectrical Impedance Analysis (SMF-BIA) |
| Electrode Method | Tetrapolar 8-Point Tactile Electrodes |
| Body Composition Calculation Method | No use of Empirical Estimation |
| Types of Result Sheet | InBody Results Sheet, InBody Results Sheet for Children, InBody Thermal Result Sheet |
| Digital Results | LCD Screen, LookinBody Web, LookinBody120 |
| Data Storage | Test results can be saved if the member ID is utilized. The InBody can save up to 100,000 results. |
| Test Mode | Self Mode, Professional Mode |
| Test Duration | About 30 Seconds |
| Weight Range | 2 - 250 kg (4.4 - 551.2 lb) |
| Height Range | 95 - 220 cm (3 ft 1.4 in - 7 ft 2.6 in) |
| Age Range | 3+ years |
| Administrator Menu | · Setup: Settings Configuration and Data Management · Troubleshooting: Additional Guidance for Using the InBody |
| USB Thumb Drive | Copy, Back Up, or Restore the InBody Test Data (which can be viewed in Excel or with LookinBody data management software). |
| Backup Data | Backup data from the device using an InBody USB or a USB thumb drive, and restore results as needed. |
| Dimensions | 356 (W) X 796 (L) X 995 (H) : mm 14.0 (W) X 31.3 (L) X 39.2 (H) : inch |
| Device Weight | 13.4 kg (29.5 lb) |
| Applied Rating Current | 300 µA (± 30 µA) |
| Operation Environment | 10 - 40 °C (50 - 104 °F), 30 - 75 % RH, 70 - 106 kPa |
| Storage Environment | -10 - 70 °C (14 - 158 °F), 10 - 80 % RH, 50 - 106 kPa (No Condensation) |
| Display Type | 480 × 800 7 inch Color TFT LCD |
| Internal Interface | Touchscreen, Keypad |
| External Interface | RS-232C 1 EA, USB HOST 2 EA, USB SLAVE 1 EA, LAN (10/100 T) 1 EA, Bluetooth 1 EA, Wi-Fi (2.4 G/5 G) 1 EA |
| Adapter | DELTA Power Input AC 100 - 240 V, 50 - 60 Hz, 1.5 A - 0.75 A Power Output DC 12 V = , 5.0 A Mean Well (GSM 40A12) Power Input AC 100 - 240 V, 50 / 60 Hz, 1.0 A - 0.5 A Power Output DC 12 V = , 3.34 A |
| Wireless Connection | Bluetooth, Wi-Fi |
| Compatible Items | Stadiometer, Blood pressure monitor, Thermal Printer (TP100), Serial Distributor (SD400), InGrip |
| Compatible Printer | Laser/Inkjet PCL 3 or above and SPL |
| Notification Sounds and Voice Guidance | Notification sounds (test in progress, saving settings, personal information, etc.) and voice guidance during the test |
| Logo Display | Name, Address, and Contact Information can be shown on the InBody Results Sheet. |
| QR Code | By scanning QR codes, you can send and verify the InBody results. |
| Language Support | InBody supports over 30 languages. |

Outputs (InBody Result Sheet)

- Results and Interpretations
- Body Composition Analysis (Total Body Water, Protein, Minerals, Body Fat Mass, Weight)
 - Muscle-Fat Analysis (Weight, Skeletal Muscle Mass, Body Fat Mass)
 - Obesity Analysis (Body Mass Index, Percent Body Fat)
 - Segmental Lean Analysis (Right Arm, Left Arm, Trunk, Right Leg, Left Leg)
 - Segmental Fat Analysis (Right Arm, Left Arm, Trunk, Right Leg, Left Leg)
 - Body Composition History (Weight, Skeletal Muscle Mass, Percent Body Fat)
 - InBody Score
 - Whole Body Phase Angle (History)
 - SMI (History)
 - Weight Control (Target Weight, Weight Control, Fat Control, Muscle Control)
 - Nutrition Evaluation (Protein, Minerals, Fat Mass)
 - Obesity Evaluation (BMI, Percent Body Fat)
 - Body Balance Evaluation (Upper, Lower, Upper-Lower)
 - Waist-Hip Ratio (Graph)
 - Visceral Fat Level (Graph)
 - Research Parameters (Skeletal Muscle Mass, Fat Free Mass, Basal Metabolic Rate, Waist-Hip Ratio, Waist Circumference, Visceral Fat Level, Obesity Degree, FFMI, FMI, SMI, SMM/WT)
 - Recommended Calorie Intake Per Day
 - Calorie Expenditure of Exercise
 - Sarcopenia Parameter (SMI, HGS)
 - Blood Pressure (Systolic, Diastolic, Pulse, Mean Artery Pressure, Pulse Pressure, Rate Pressure Device)
 - QR Code
 - Results Interpretation QR Code
 - Whole Body Phase Angle (50 kHz)
 - Impedance (Each segment and each frequency)

Outputs (InBody Result Sheet for Children)

- Results and Interpretations
- Body Composition Analysis (Total Body Water, Protein, Minerals, Body Fat Mass, Weight)
 - Muscle-Fat Analysis (Weight, Skeletal Muscle Mass, Body Fat Mass)
 - Obesity Analysis (Body Mass Index, Percent Body Fat)
 - Growth Graph (Height, Weight, BMI)
 - Body Composition History (Height, Weight, Skeletal Muscle Mass, Percent Body Fat)
 - Whole Body Phase Angle (History)
 - SMI (History)
 - Growth Score
 - Weight Control (Target Weight, Weight Control, Fat Control, Muscle Control)
 - Obesity Evaluation (BMI, Percent Body Fat)
 - Nutrition Evaluation (Protein, Minerals, Fat Mass)
 - Body Balance (Upper, Lower, Upper-Lower)
 - Research Parameters (Skeletal Muscle Mass, Fat Free Mass, Basal Metabolic Rate, Child Obesity Degree, FFMI, FMI, SMI, SMM/WT)
 - Sarcopenia Parameter
 - Blood Pressure (Systolic, Diastolic, Pulse, Mean Artery Pressure, Pulse Pressure, Rate Pressure device)
 - QR Code
 - Results Interpretation QR Code
 - Whole Body Phase Angle (50 kHz)
 - Impedance (Each segment and each frequency)

Outputs (InBody Thermal Result Sheet)

- Total Body Water, Protein, Minerals, Weight, Muscle Mass, Body Fat Mass, Percent Body Fat, BMI, Basal Metabolic Rate, Waist-Hip Ratio, Waist Circumference, Visceral Fat Level, FFMI, FMI, SMI, SMM/WT, Segmental Lean Analysis (Right Arm, Left Arm, Trunk, Right Leg, Left Leg), Segmental Fat Analysis (Right Arm, Left Arm, Trunk, Right Leg, Left Leg), InBody Score, Fat Control, Muscle Control, Whole Body Phase Angle (50 kHz), Impedance (Each segment and each frequency)

* The above content is subject to change without prior notice for the purpose of improving device appearance and performance.
* Note that this is a medical device, and use it with proper care and knowledge of its precautions and instructions.
* The results about Blood Pressure or Hand Grip Strength are only available when integrated with InBody Blood Pressure Monitor (BPBIO Series) or InBody Handgrip Dynamometer (InGrip).
* "QR Code" is registered trademark of DENSO WAVE INCORPORATED.

InBody

InBody HQ [KOREA]

InBody Co., Ltd.
InBody Bldg., 625, Eonju-ro, Gangnam-gu, Seoul
06106 Republic of Korea
TEL: +82-2-501-3939 FAX: +82-2-6919-2417
Website: inbody.com
E-mail: info@inbody.com

InBody China [CHINA]

Biospace China Co., Ltd.
Room 306b, 307a, 307b, 308, MT2 Office Building,
No. 3999 Hongxin Road, Minhang District, Shanghai
TEL: +61-7-5681-1900 FAX: +86-21-6443-9706
Website: inbodychina.com
E-mail: info@inbodychina.com

InBody Oceania [AUSTRALIA]

InBody Oceania Pty Ltd.
U2/82-86 Minnie Street, Southport, Queensland
TEL: +61-7-5681-1900 FAX: +61-7-5681-1900
Website: au.inbody.com
Email: oceania@inbody.com

InBody USA [USA]

Biospace Inc. dba InBody
13850 Cerritos Corporate Dr. Unit C Cerritos,
CA 90703 USA
TEL: +1-323-932-6503 FAX: +1-323-952-5009
Website: inbodyusa.com
E-mail: info.us@inbody.com

InBody Europe B.V. [NETHERLANDS]

InBody Europe B.V.
Gyroscoopweg 122, 1042 AZ, Amsterdam,
The Netherlands
TEL: +31-20-238-6080 FAX: +31-6-5734-1858
Website: nl.inbody.com
E-mail: info.eu@inbody.com

Biospace Latin America [MÉXICO]

Insurgentes Sur 1457, Piso 15 Int.2. Col. Insurgentes
Mixcoac, Alcatla Benito Juarez, C.P. 03920, Ciudad
de México, México
TEL: +52-55-5025-0147
Website: inbodymexico.com
E-mail: info.mx@inbody.com

InBody BWA Inc. [USA]

InBody BWA Inc.
2550 Eisenhower Avenue, Suite C 209, Audubon, PA 19403
TEL: +1-610-348-7745
Website: inbodybwa.com
E-mail: bwainquiries@inbody.com

InBody Europe B.V. Niederlassung

Deutschland [GERMANY]
InBody Europe B.V.
Mergenthalerallee 15-21, 65760 Eschborn, Germany
TEL: +49-6196-76-916-62 FAX: +49-6196-76-916-11
Website: de.inbody.com
E-mail: erfolg@inbody.com

InBody Asia [MALAYSIA & SINGAPORE]

InBody Asia Sdn. Bhd.
Unit 3A-11, Oval Damansara, 685 Jalan Damansara
Kuala Lumpur, WP KL 60000 Malaysia
TEL: +60-3-7732-0790 FAX: +60-3-7733-0790
Website: inbodyasia.com
E-mail: info@inbodyasia.com

InBody Japan [JAPAN]

InBody Japan Inc.
Tani Bldg., 1-28-6, Kameido, Koto-ku, Tokyo
136-0071 Japan
TEL: +81-3-5875-5780 FAX: +81-3-5875-5781
Website: inbody.co.jp
E-mail: inbody@inbody.co.jp

InBody UK [UNITED KINGDOM]

Orega, Belmont Road, Uxbridge, UB8 1HE,
United Kingdom
TEL: +44-1530-569620
Website: uk.inbody.com
E-mail: uk@inbody.com

InBody India [INDIA]

InBody India Pvt.Ltd.
57/57 A, 1st Floor, Raj Industrial Complex, Military
Road, Marol, Andheri (East), Mumbai- 400059,
Maharashtra, India
TEL: +91-22-6223-1911
Website: inbody.in
E-mail: india@inbody.com

Certificates



Awards



For more details about the patents that we acquired, please visit our website or refer to the patent gazette of intellectual property office of each country. (Korea, U.S, China, Japan)